

RoboSep™-C Human CD4+ T Cell Isolation Kit

For processing 1 x 10¹⁰ cells

Catalog #100-0200

Negative Selection

Document #1000008421 | Version 03



Scientists Helping Scientists™ | WWW.STEMCELL.COM

TOLL FREE PHONE 1 800 667 0322 • PHONE +1 604 877 0713

INFO@STEMCELL.COM • TECHSUPPORT@STEMCELL.COM

FOR GLOBAL CONTACT DETAILS VISIT OUR WEBSITE

Description

Isolate untouched and highly purified CD4+ T cells from fresh human peripheral blood leukopaks using RoboSep™-C (Catalog #100-0185/100-0186) for automated immunomagnetic negative selection.

- Fully automated large-scale isolation in a closed system
- Up to 98% purity with high recovery
- Untouched, viable cells

This kit targets non-CD4+ T cells for removal with antibodies recognizing specific cell surface markers. Using RoboSep™-C in a fully automated protocol, unwanted cells are labeled with antibodies and magnetic particles, and separated without columns using a RoboSep™-C magnet. Desired cells are washed and concentrated by RoboSep™-C and transferred to a final product bag. Isolated cells are immediately available for downstream applications such as flow cytometry, culture, or cryopreservation.

Component Descriptions

COMPONENT NAME	COMPONENT #	QUANTITY	STORAGE	SHELF LIFE	FORMAT
RoboSep™-C Human CD4+ T Cell Isolation Cocktail	300-0107	1 x 10 mL	Store at 2 - 8°C. Do not freeze.	Stable until expiry date (EXP) on label.	A combination of monoclonal antibodies in PBS.
RoboSep™-C Dextran RapidSpheres™ 30106	300-0106	1 x 10 mL	Store at 2 - 8°C. Do not freeze.	Stable until expiry date (EXP) on label.	A suspension of magnetic particles in water.

PBS - phosphate-buffered saline

Components may be shipped at room temperature (15 - 25°C) but should be stored as indicated above.

Materials Required But Not Included

PRODUCT NAME	CATALOG #
RoboSep™-C	100-0185 OR 100-0186
RoboSep™-C Tubing Set	200-0090
RoboSep™-C PBS/EDTA Buffer	100-0188
Fetal bovine serum (FBS)	e.g. 100-0179
Tube sealer	e.g. Sebra 2600-1105
20 mm vial access devices	e.g. Yukon Medical YM-038
Luer lock syringes	e.g. BD 309604/309653

Sample Preparation

For available fresh human peripheral blood leukopaks, see www.stemcell.com/primarycells (e.g. Catalog #70500).

1. Determine the number of nucleated cells in the leukopak. Ensure the number of cells is between 2.5 and 20 x 10⁹ cells. For > 20 x 10⁹ cells, split the sample into multiple runs.

NOTE: Each RoboSep™-C Human CD4+ T Cell Isolation Kit processes up to 10 x 10⁹ cells. For leukopaks containing > 10 x 10⁹ cells, multiple kits are required.

2. Using aseptic technique, transfer sample into Sample Bag 1 provided in the RoboSep™-C Tubing Set, as follows:
 - a. Spike the line of Sample Bag 1 containing the in-line blood filter into a spike port of the leukopak bag.
 - b. Drain the contents of the leukopak bag into Sample Bag 1 by gravity. Flick the blood filter to minimize retention of sample volume in the line.
 - c. Close the pinch clamp on the Sample Bag 1 line and use a tube sealer to seal off the tubing at a site between the blood filter and the sample bag. Remove and discard the sealed-off tubing.
3. Follow on-screen prompts to load Sample Bag 1 onto the instrument (Table 1).

Recommended Medium

Use aseptic technique to prepare recommended medium (RoboSep™-C PBS/EDTA Buffer + 2% FBS), as follows:

- Using a syringe, inject 60 mL of FBS into the RoboSep™-C PBS/EDTA Buffer bag via the luer injection port on the bag.
- Invert bag several times to mix thoroughly.
NOTE: If not used immediately, store recommended medium at 2 - 8°C. Do not exceed the shelf life of the individual components. Warm to room temperature (15 - 25°C) before use.

Directions for Use – Fully Automated RoboSep™ Protocol

See pages 1 and 2 for Sample Preparation and Recommended Medium. Refer to Table 1 for detailed instructions regarding the RoboSep™-C procedure.

For RoboSep™-C setup instructions, refer to the RoboSep™-C User Reference Manual (Document #1000008334), available at www.stemcell.com or contact us to request a copy. Use aseptic technique for all steps.

Table 1. RoboSep™-C Human CD4+ T Cell Isolation Kit Protocol

STEP	INSTRUCTIONS	RoboSep™-C (Catalog #100-0185/100-0186)
1	Select kit.	Human CD4+ T Cell Isolation 100-0200
2	Select protocol corresponding to number of cells in sample.	<ul style="list-style-type: none"> • 2.5 to < 5 x 10⁹ cells • 5 to < 10 x 10⁹ cells • 10 to 20 x 10⁹ cells
3	Install Tubing Set.	Follow on-screen prompts.
4	Connect Recommended Medium: <ul style="list-style-type: none"> • Remove cap from the primary buffer spike on the Tubing Set and connect it to the Recommended Medium Bag. • Squeeze bag to prime filter. • Hang Recommended Medium Bag on Weight Scale 7. 	Follow on-screen prompts.
5	Add Isolation Cocktail to Process Bag 3: <ul style="list-style-type: none"> • Attach a 20 mm vial access device to the cocktail vial. • Connect a syringe to the vial access device, invert the vial, and draw up the indicated volume of cocktail plus a 2 mL bolus of air. Disconnect the syringe from the vial. • Remove Process Bag 3 from Weight Scale 3. • Remove cap from the injection port on Process Bag 3. • With the injection port pointing up, inject the Isolation Cocktail followed by the bolus of air into Process Bag 3. • Invert bag to mix and re-hang on Weight Scale 3. 	Use 1 mL cocktail per 10 ⁹ cells (e.g. for 10 x 10 ⁹ cells, inject 10 mL of cocktail).
6	Add Dextran RapidSpheres™ to Process Bag 2: <ul style="list-style-type: none"> • Vortex RapidSpheres™ for 30 seconds. Particles should appear evenly dispersed. • Attach a 20 mm vial access device to the particle vial. • Connect a syringe to the vial access device, invert the vial, and draw up the indicated volume of particles plus a 2 mL bolus of air. Disconnect the syringe from the vial. • Remove Process Bag 2 from Weight Scale 2. • Remove cap from the injection port on Process Bag 2. • With the injection port pointing up, inject the particles followed by the bolus of air into Process Bag 2. • Invert bag to mix and re-hang on Weight Scale 2. 	Use 1 mL particles per 10 ⁹ cells (e.g. for 10 x 10 ⁹ cells, inject 10 mL of particles).
7	Connect Sample Bag 1: <ul style="list-style-type: none"> • Remove cap from a spike port on Sample Bag 1. • Remove cap from the Start Sample Spike and connect it to Sample Bag 1. • Hang Sample Bag 1 on Weight Scale 1. 	Follow on-screen prompts.
8	Collect isolated cells when the run is complete: <ul style="list-style-type: none"> • Close pinch clamp below Process Bag 4. • Seal the tubing below pinch clamp using a tube sealer and remove Process Bag 4 containing the isolated cells. 	Isolated cells are in Process Bag 4 on Weight Scale 4.

Notes and Tips

TROUBLESHOOTING


For troubleshooting tips, refer to the RoboSep™-C User Reference Manual (Document #10000008334), available at www.stemcell.com or contact us to request a copy.

ASSESSING PURITY

For purity assessment of CD4+ T cells (CD3+CD4+) by flow cytometry, use the following fluorochrome-conjugated antibody clones:

- Anti-Human CD3 Antibody, Clone UCHT1 (Catalog #60011), and
- Anti-Human CD4 Antibody, Clone OKT4 (Catalog #60016)

Data

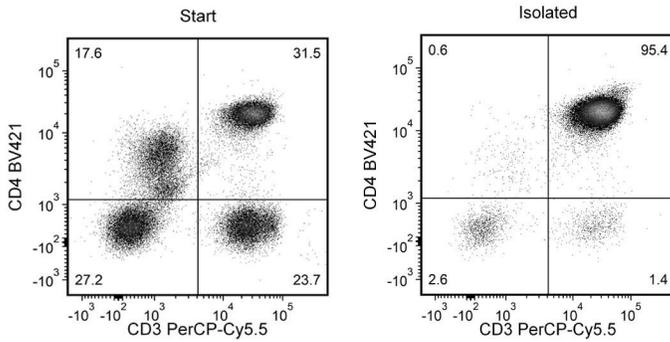

Starting with a fresh human peripheral blood leukopak, the CD4+ T cell content (CD3+CD4+) of the isolated fraction is typically $95.7 \pm 2.8\%$ (mean \pm SD). In the above example, the purities of the start and final isolated fractions are 31.5% and 95.4%, respectively.

PRODUCTS ARE FOR RESEARCH USE ONLY AND NOT INTENDED FOR HUMAN OR ANIMAL DIAGNOSTIC OR THERAPEUTIC USES UNLESS OTHERWISE STATED. FOR ADDITIONAL INFORMATION ON QUALITY AT STEMCELL, REFER TO WWW.STEMCELL.COM/COMPLIANCE.

Copyright © 2021 by STEMCELL Technologies Inc. All rights reserved including graphics and images. STEMCELL Technologies & Design, STEMCELL Shield Design, Scientists Helping Scientists, EasySep, RapidSpheres, and RoboSep are trademarks of STEMCELL Technologies Canada Inc. All other trademarks are the property of their respective holders. While STEMCELL has made all reasonable efforts to ensure that the information provided by STEMCELL and its suppliers is correct, it makes no warranties or representations as to the accuracy or completeness of such information.